

COMPONENTS

Kit Component	Amount
96-well plate pre-coated with anti-human IGF-2 antibody	1 Plate
Protein Standard: Lyophilized recombinant human IGF-2	2 tubes, 10 ng/tube
Sample Diluent Buffer	30 ml
Biotinylated Antibody (Anti-human IGF-2)	130 µl (100x)
Antibody Diluent Buffer	12ml
Avidin-Biotin-Peroxidase Complex (ABC) Solution	130 µl (100x)
ABC Diluent Buffer	12 ml
Tetramethylbenzidine (TMB) Color Developing Agent	10 ml
TMB Stop Solution	10 ml


Washing Buffer (not provided): TBS or PBS

0.01M TBS: Add 1.2g Tris, 8.5g NaCl; 450µl of purified acetic acid or 700µl of concentrated hydrochloric acid to 900ml H₂O and adjust pH to 7.2-7.6. Adjust the total volume to 1L.

0.01M PBS: Add 8.5g sodium chloride, 1.4g Na₂HPO₄ and 0.2g NaH₂PO₄ to 900ml distilled H₂O and adjust pH to 7.2-7.6. Adjust the total volume to 1L.

Storage

Store at 4°C. Cell Applications, Inc. recommends using the kit within 6 months of order.

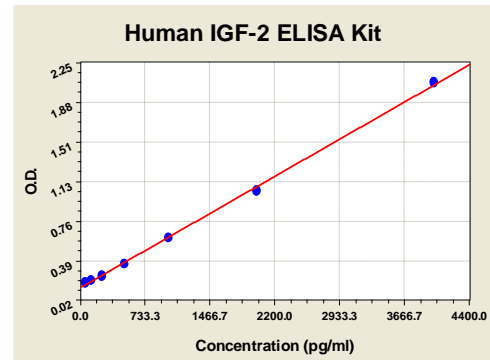

X	pg/ml	0.0	62.5	125	250	500	1000	2000	4000	
Y	O.D.	0.0450	0.153	0.187	0.199	0.246	0.354	0.601	1.051	2.062

Figure 1: IGF-2 Standard Curve. Using the Human IGF-2 ELISA Kit, O.D. data was graphed against IGF-2 protein concentration. The TMB reaction was incubated at 37°C for 15 min.

BACKGROUND

Insulin-like growth factor II (IGF-II) plays a key role in mammalian growth, influencing fetal cell division and differentiation and possibly metabolic regulation. The mature 67 amino acid peptide shares sequence homology with both insulin and IGF-I. The liver is the main endocrine source of IGFs, but autocrine/paracrine activity is found in most tissues. IGF-II binds to two types of receptors. The IGF-I receptor that is a tyrosine kinase and closely related with the insulin receptor and the IGF-II/mannose 6-phosphate receptor that is identical with the cation-independent mannose 6-phosphate receptor. The mitogenic and metabolic actions of IGF-II are propagated by the IGF-I receptor. In contrast, the receptor, that target lysosomal enzymes from the Golgi apparatus or the plasma membrane to the lysosomes, mediates the rapid internalization and degradation of IGF-II.¹ IGF-II is expressed at high levels during fetal life and it is a major growth factor for the fetus in rodents. The developmental profiles and tissue distribution of the IGF-I and the maternally imprinted receptors both parallel that of IGF-II. In this scenario IGF-II promotes the growth of the embryo through the IGF-I receptor, whereas the receptor balance the activity by controlling the extracellular level of IGF-II. Binding proteins may both localize IGFs to the receptors and regulate their activities.² The IGF-II gene is coupled to the insulin gene and paternally imprinted. Relaxation of IGF2 imprinting occurs in the Beckwith–Wiedemann syndrome of somatic overgrowth, sporadic Wilms' tumor and a number of other cancers. In the general adult population, the IGF2-INS gene cluster may also influence body weight, in which case IGF-II function could become a target for therapeutic intervention in obesity.³

References

- Nielsen, F.C. et al: Prog. Growth Factor Res. 4:257-90, 1992
- Sandberg, A.C. et al: Neurosci. Let. 93:114-9, 1988
- LeRoith, D. & Bondy, C.: Growth Factors and Cytokines Health Dis. 1:1-26, 1996

ELISA OVERVIEW


Cell Applications ELISA Kits are based on standard sandwich enzyme-linked immunosorbent assay technology. Freshly prepared standards, samples, and solutions are recommended for best results.

- Prepare test samples.
- Prepare a protein standard of the target protein.
- Add test samples and standards to the pre-coated 96-well plate. Do not wash.
- Add biotinylated detection antibodies. Wash.
- Add Avidin-Biotin-Peroxidase Complex (ABC) Solution. Wash.
- Add Tetramethylbenzidine (TMB) Color Developing Agent, containing HRP substrate.
- Add TMB Stop Solution
- Subject the plate to analysis.

NOTES:

- Before using the kit, quick spin tubes to bring down all solution to the bottom of tube.
- Duplicate assay wells are recommended for both standard and sample testing.
- Do not let the 96-well plate dry, this will lead to inactivation of plate components.
- When diluting samples and reagents, ensure that they are mixed completely and evenly.
- Pre-warm diluted ABC and TMB solutions at 37°C for 30 min before use to avoid variable temperature effects.
- For washes, use TBS or PBS. Do not touch well walls.
- A protein standard is included in the kit. A protein standard detection curve should be generated with each experiment, no more than 2 hours prior to the experiment.
- The user will determine sample dilution fold by estimation of target protein amount in samples.

FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR CLINICAL USE.



PROTOCOL

I. Plate Washing

Discard the solution in the plate without touching the side walls. Blot the plate onto paper towels or other absorbent material. Soak each well with at least 0.3 ml PBS or TBS buffer for 1–2 minutes. Repeat this process two additional times for a total of three washes.

II. Preparation of Test Samples

Test Sample Processing

- **Cell culture supernate, tissue lysate or body fluids:** Remove particulates by centrifugation.
- **Serum:** Allow the serum to clot in a serum separator tube (about 2 hours) at room temperature. Centrifuge at approximately 1000 X g for 10 min.
- **Plasma:** Collect plasma using heparin, EDTA as an anticoagulant. Centrifuge for 15 min at 1000 x g within 30 min of collection. Analyze immediately or aliquot and store frozen at -20°C. Citrate is not recommended as the anticoagulant.

Sample Dilution Guideline

Estimate the concentration of the target protein in the sample and select a proper dilution factor such that the diluted target protein concentration falls within the standard curve range. Depending on the sample, several trial dilutions may be necessary. Dilute the sample using the provided diluent buffer, mixing well. Suggested working dilutions of samples are as follows:

Target Protein Concentration Range	Sample Working Dilution	Sample Vol.	Diluent Buffer Vol.
40-400 ng/ml	1:100	1 µl	99 µl
4-40 ng/ml	1:10	10 µl	90 µl
62.5-4000 pg/ml	1:2	50 µl	50 µl
≤62.5 pg/ml	n/a	100µl	n/a

If samples will be assayed within 24 hours, store at 2-8°C. For long-term storage, aliquot and freeze samples at -20°C. Avoid repeated freeze-thaw cycles.

IMPORTANT: Bovine serum in cell culture media may contain IGF-2. To account for the possibility of IGF-2 in serum-based media, add an equivalent amount of media as the Test Samples (after dilution) to the Sample Diluent Buffer for analysis.

III. Preparation of Reagents

Reconstitution of the Standard

The standard solutions should be prepared no more than 2 hours prior to the experiment. Two tubes of the standard are included in each kit. Use one tube for each experiment.

1. 10,000pg/ml of human IGF-2 standard solution: Add 1 ml sample diluent buffer into one tube, keep the tube at room temperature for 10 min and mix thoroughly.
2. 4000pg/ml of human IGF-2 standard solution: Add 0.4 ml of the above 10ng/ml IGF-2 standard solution into 0.6 ml sample diluent buffer and mix thoroughly.
3. 2000pg/ml→62.5pg/ml of human IGF-2 standard solutions: Label 6 Eppendorf tubes with 2000pg/ml, 1000pg/ml, 500pg/ml, 250pg/ml, 125pg/ml, 62.5pg/ml, respectively. Aliquot 0.3 ml of the sample diluent buffer into each tube. Add 0.3 ml of the above 4000pg/ml IGF-2 standard solution into 1st tube and mix. Transfer 0.3 ml from 1st tube to 2nd tube and mix. Transfer 0.3 ml from 2nd tube to 3rd tube and mix, and so on.

Preparation of Biotinylated Antibody Working Solution

The solution should be prepared no more than 2 hours prior to the experiment.

1. The total volume should be: 0.1ml/well x (the number of wells). (Allowing 0.1-0.2 ml more than total volume)
2. Biotinylated antibody should be diluted in 1:100 with the antibody diluent buffer and mixed thoroughly.

Preparation of the Avidin-Biotin-Peroxidase Complex (ABC) Working Solution

The solution should be prepared no more than 1 hour prior to the experiment.

1. The total volume should be: 0.1ml/well x (the number of wells). (Allowing 0.1-0.2 ml more than total volume)
2. Avidin- Biotin-Peroxidase Complex (ABC) should be diluted in 1:100 with the ABC dilution buffer and mixed thoroughly.

IV. ELISA

The ABC working solution and TMB color developing agent must be kept warm at 37°C for 30 min before use. When diluting samples and reagents, they must be mixed completely and evenly. A standard detection curve should be prepared for each experiment. The user will decide sample dilution fold by crude estimation of target protein amount in samples.

1. Aliquot 0.1ml per well of the 4000pg/ml, 2000pg/ml, 1000pg/ml, 500pg/ml, 250pg/ml, 125pg/ml, 62.5pg/ml human IGF-2 standard solutions into the precoated 96-well plate. Add 0.1ml of the sample diluent buffer into the control well (Zero well). Add 0.1ml of each properly diluted sample of human sera, plasma, body fluids, tissue lysates or cell culture supernatants to each empty well. See "Sample Dilution Guideline" above for details. We recommend that each human IGF-2 standard solution and each sample is measured in duplicate.
2. Seal the plate with the cover and incubate at 37°C for 90 min.
3. Remove the cover, discard plate content, and blot the plate onto paper towels or other absorbent material. Do NOT let the wells completely dry at any time.
4. Add 0.1ml of biotinylated anti-human IGF-2 antibody working solution into each well and incubate the plate at 37°C for 60 min.
5. Wash the plate three times with 0.01M TBS or 0.01M PBS, and each time let washing buffer stay in the wells for 1 min. Discard the washing buffer and blot the plate onto paper towels or other absorbent material.
6. Add 0.1ml of prepared ABC working solution into each well and incubate the plate at 37°C for 30 min.
7. Wash plate 5 times with 0.01M TBS or 0.01M PBS, and each time let washing buffer stay in the wells for 1-2 min. Discard the washing buffer and blot the plate onto paper towels or other absorbent material.
8. Add 90 µl of prepared TMB color developing agent into each well and incubate plate at 37°C for 25-30 min (shades of blue can be seen in the wells with the four most concentrated human IGF-2 standard solutions; the other wells show no obvious color).
9. Add 0.1ml of prepared TMB stop solution into each well. The color changes into yellow immediately.
10. Read the O.D. absorbance at 450nm in a microplate reader within 30 min after adding the stop solution.

V. Calculating Protein Concentration

- For all wells, determine O.D.450(Relative):

$$\text{O.D.450(Relative)} = \text{O.D.450(Reading)} - \text{O.D.450(Blank)}$$
- Plot the standard curve:
 Plot O.D.450(Relative) of each standard solution (Y) vs. the respective concentration of the standard solution (X). See **Figure 1** for a typical standard curve.
- The target protein concentration in samples can be interpolated from the standard curve. Multiply the interpolated concentration by the dilution factor to obtain the target protein concentration in the sample.

FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR CLINICAL USE.

