

COMPONENTS

| Kit Component | Amount |
|--|---------------------|
| 96-well plate precoated with anti-mouse MCP-1 antibody | 1 Plate |
| Protein Standard: Lyophilized recombinant mouse MCP-1 | 2 tubes, 10 ng/tube |
| Sample Diluent Buffer | 30 ml |
| Biotinylated Antibody (Anti-mouse MCP-1) | 130 µl (100x) |
| Antibody Diluent Buffer | 12ml |
| Avidin-Biotin-Peroxidase Complex (ABC) Solution | 130 µl (100x) |
| ABC Diluent Buffer | 12 ml |
| Tetramethylbenzidine (TMB) Color Developing Agent | 10 ml |
| TMB Stop Solution | 10 ml |


Washing Buffer (not provided): TBS or PBS

0.01M TBS: Add 1.2g Tris, 8.5g NaCl; 450µl of purified acetic acid or 700µl of concentrated hydrochloric acid to 900ml H₂O and adjust pH to 7.2-7.6. Adjust the total volume to 1L.

0.01M PBS: Add 8.5g sodium chloride, 1.4g Na₂HPO₄ and 0.2g NaH₂PO₄ to 900ml distilled H₂O and adjust pH to 7.2-7.6. Adjust the total volume to 1L.

Storage

Store at 4°C. Cell Applications, Inc. recommends using the kit within 6 months of order.

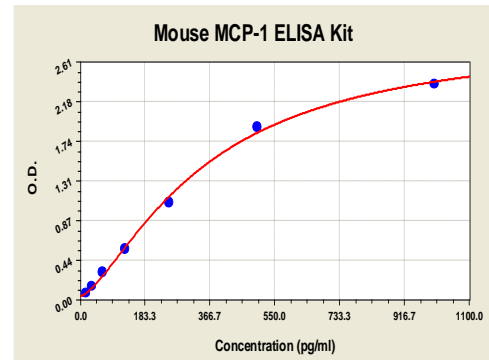

| X | pg/ml | 0.0 | 156 | 313 | 625 | 125 | 250 | 500 | 1000 |
|---|---------|-------|-------|-------|-------|-------|-------|-------|-------|
| Y | O.D.450 | 0.000 | 0.077 | 0.158 | 0.310 | 0.569 | 1.077 | 1.903 | 2.376 |

Figure 1: MCP-1 Standard Curve. Using the Mouse MCP-1 ELISA Kit, O.D. data was graphed against MCP-1 protein concentration. The TMB reaction was incubated at 37°C for 25 min.

BACKGROUND

Monocyte chemoattractant protein-1 (MCP-1) was the first CC chemokine identified. Human MCP-1 is composed of 76 amino acids and is 13 kDa in size. MCP subfamily composed of at least four members (MCP-1, -2, -3, and -4).¹ MCP-1 is produced by a variety of cell types, either constitutively or after induction by oxidative stress, cytokines, or growth factors. Many activities have been assigned to MCP-1, including induction of migration of macrophages/monocytes, memory/activated T cells and NK cells and activation of mast cells. MCP-1 mediates its cellular effects primarily through its binding to CCR2, which exists in A and B forms that arise via alternative splicing of the carboxyl-terminal tail. Unlike MCP-1, CCR2 expression is relatively restricted to certain types of cells. CCR2A is the major isoform expressed by mononuclear cells and vascular smooth muscle cells, while monocytes and activated NK cells, express predominantly the CCR2B isoform. It is possible that CCR2A and CCR2B may activate different signaling pathway and exert different actions. In addition, there may be another alternative MCP-1 receptor which may be important in mediating some of the effects of MCP-1 in atherosclerotic arteries and in other inflammatory processes.² Both MCP-1 and its receptor CCR2 have been demonstrated to be induced and involved in a variety of diseases. Analysis of the signal transduction pathways triggered by MCP-1 has revealed that it induces a pertussis toxin (PTX)-sensitive rise of intracellular calcium, inhibition of adenylyl cyclase, phospholipase C activation, activation of extracellular signal-related kinases (ERKs) and the 2 stress-activated protein kinases (SAPKs), JNK1 and P38, stimulation of 2 separate PI 3-kinase isoforms, namely p85/p110 PI3-kinase (PI3-K) and PI3K-C2alpha. Recently, analysis of signaling events in human monocytic cells has shown that MCP-1 triggers tyrosine phosphorylation and activation of the JAK2/STAT3 pathway in a PTX-independent manner.³

References

- Gerard, C. & and Rollins, B.J.: Nature Immunol. 2:108-115, 2001
- Schechter, S.D. et al: J. Leuk. Biol. 75:1079-1085, 2004
- Cambien, B. et al: Blood 97:359-66, 2001

ELISA OVERVIEW


Cell Applications ELISA Kits are based on standard sandwich enzyme-linked immunosorbent assay technology. Freshly prepared standards, samples, and solutions are recommended for best results.

- Prepare test samples.
- Prepare a protein standard of the target protein.
- Add test samples and standards to the pre-coated 96-well plate. Do not wash.
- Add biotinylated detection antibodies. Wash.
- Add Avidin-Biotin-Peroxidase Complex (ABC) Solution. Wash.
- Add Tetramethylbenzidine (TMB) Color Developing Agent, containing HRP substrate.
- Add TMB Stop Solution
- Subject the plate to analysis.

NOTES:

- Before using the kit, quick spin tubes to bring down all solution to the bottom of tube.
- Duplicate assay wells are recommended for both standard and sample testing.
- Do not let the 96-well plate dry, this will lead to inactivation of plate components.
- When diluting samples and reagents, ensure that they are mixed completely and evenly.
- Pre-warm diluted ABC and TMB solutions at 37°C for 30 min before use to avoid variable temperature effects.
- For washes, use TBS or PBS. Do not touch well walls.
- A protein standard is included in the kit. A protein standard detection curve should be generated with each experiment, no more than 2 hours prior to the experiment.
- The user will determine sample dilution fold by estimation of target protein amount in samples.

FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR CLINICAL USE.



PROTOCOL

I. Plate Washing

Discard the solution in the plate without touching the side walls. Blot the plate onto paper towels or other absorbent material. Soak each well with at least 0.3 ml PBS or TBS buffer for 1–2 minutes. Repeat this process two additional times for a total of three washes.

II. Preparation of Test Samples

Test Sample Processing

- **Cell culture supernate, tissue lysate or body fluids:** Remove particulates by centrifugation.
- **Serum:** Allow the serum to clot in a serum separator tube (about 2 hours) at room temperature. Centrifuge at approximately 1000 X g for 10 min.
- **Plasma:** Collect plasma using EDTA as an anticoagulant. Centrifuge for 20 min at 2000 x g within 30 min of collection. Analyze immediately or aliquot and store frozen at -20°C.

Sample Dilution Guideline

Estimate the concentration of the target protein in the sample and select a proper dilution factor such that the diluted target protein concentration falls within the standard curve range. Depending on the sample, several trial dilutions may be necessary. Dilute the sample using the provided diluent buffer, mixing well. Suggested working dilutions of samples are as follows:

| Target Protein Concentration Range | Sample Working Dilution | Sample Vol. | Diluent Buffer Vol. |
|------------------------------------|-------------------------|-------------|---------------------|
| 10-100 ng/ml | 1:100 | 1 µl | 99 µl |
| 4110 ng/ml | 1:10 | 10 µl | 90 µl |
| 15.6-1000 pg/ml | 1:2 | 50 µl | 50 µl |
| ≤15.6 pg/ml | n/a | 100µl | n/a |

If samples will be assayed within 24 hours, store at 2-8°C. For long-term storage, aliquot and freeze samples at -20°C. Avoid repeated freeze-thaw cycles.

III. Preparation of Reagents

Reconstitution of the Standard

The standard solutions should be prepared no more than 2 hours prior to the experiment. Two tubes of the standard are included in each kit. Use one tube for each experiment.

1. 10,000pg/ml of mouse Fractalkine standard solution: Add 1 ml sample diluent buffer into one tube, keep the tube at room temperature for 10 min and mix thoroughly.
2. 1000pg/ml of mouse MCP-1 standard solution: Add 0.1 ml of the above 10000pg/ml MCP-1 standard solution into 0.9 ml sample diluent buffer and mix thoroughly.
3. 500pg/ml→15.6pg/ml of mouse MCP-1 standard solutions: Label 6 Eppendorf tubes with 500pg/ml, 250pg/ml, 125pg/ml, 62.5pg/ml, 31.3pg/ml, 15.6pg/ml, respectively. Aliquot 0.3 ml of the sample diluent buffer into each tube. Add 0.3 ml of the above 10, 000pg/ml MCP-1 standard solution into 1st tube and mix. Transfer 0.3 ml from 1st tube to 2nd tube and mix. Transfer 0.3 ml from 2nd tube to 3rd tube and mix, and so on.

Preparation of Biotinylated Antibody Working Solution

The solution should be prepared no more than 2 hours prior to the experiment.

1. The total volume should be: 0.1ml/well x (the number of wells). (Allowing 0.1-0.2 ml more than total volume)
2. Biotinylated antibody should be diluted in 1:100 with the antibody diluent buffer and mixed thoroughly.

Preparation of the Avidin-Biotin-Peroxidase Complex (ABC) Working Solution

The solution should be prepared no more than 1 hour prior to the experiment.

1. The total volume should be: 0.1ml/well x (the number of wells). (Allowing 0.1-0.2 ml more than total volume)
2. Avidin- Biotin-Peroxidase Complex (ABC) should be diluted in 1:100 with the ABC dilution buffer and mixed thoroughly.

IV. ELISA

The ABC working solution and TMB color developing agent must be kept warm at 37°C for 30 min before use. When diluting samples and reagents, they must be mixed completely and evenly. A standard detection curve should be prepared for each experiment. The user will decide sample dilution fold by crude estimation of target protein amount in samples.

1. Aliquot 0.1ml per well of the 1000pg/ml, 500pg/ml, 250pg/ml, 125pg/ml, 62.5pg/ml, 31.3pg/ml, 15.6pg/ml mouse MCP-1 standard solutions into the precoated 96-well plate. Add 0.1ml of the sample diluent buffer into the control well (Blank well). Add 0.1ml of each properly diluted sample of mouse sera, plasma, body fluids, tissue lysates or cell culture supernatants to each empty well. See "Sample Dilution Guideline" for details. We recommend that each mouse MCP-1 standard solution and each sample is measured in duplicate.
2. Seal the plate with the cover and incubate at 37°C for 90 min.
3. Remove the cover, discard plate content, and blot the plate onto paper towels or other absorbent material. Do NOT let the wells completely dry at any time.
4. Add 0.1ml of biotinylated anti-mouse MCP-1 antibody working solution into each well and incubate the plate at 37°C for 60 min.
5. Wash plate 3 times with 0.01M TBS or 0.01M PBS, and each time let washing buffer stay in the wells for 1 min. Discard the washing buffer and blot the plate onto paper towels or other absorbent material. (**Plate Washing Method:** Discard the solution in the plate without touching the side walls. Blot the plate onto paper towels or other absorbent material. Soak each well with at least 0.3 ml PBS or TBS buffer for 1–2 minutes. Repeat this process two additional times for a total of THREE washes. Note: For automated washing, aspirate all wells and wash THREE times with PBS or TBS buffer, overfilling wells with PBS or TBS buffer. Blot the plate onto paper towels or other absorbent material.)
6. Add 0.1ml of prepared ABC working solution into each well and incubate the plate at 37°C for 30 min.
7. Wash plate 5 times with 0.01M TBS or 0.01M PBS, and each time let washing buffer stay in the wells for 1-2 min. Discard the washing buffer and blot the plate onto paper towels or other absorbent material. (See Step 5 for plate washing method).
8. Add 90 µl of prepared TMB color developing agent into each well and incubate plate at 37°C in dark for 25-30 min (**Note:** For reference only, the optimal incubation time should be determined by end user. And the shades of blue can be seen in the wells with the four most concentrated mouse MCP-1 standard solutions; the other wells show no obvious color).
9. Add 0.1ml of prepared TMB stop solution into each well. The color changes into yellow immediately.
10. Read the O.D. absorbance at 450nm in a microplate reader within 30 min after adding the stop solution.

V. Calculating Protein Concentration

- For all wells, determine O.D.450(Relative):

$$\text{O.D.450(Relative)} = \text{O.D.450(Reading)} - \text{O.D.450(Blank)}$$
- Plot the standard curve:
 Plot O.D.450(Relative) of each standard solution (Y) vs. the respective concentration of the standard solution (X). See **Figure 1** for a typical standard curve.
- The target protein concentration in samples can be interpolated from the standard curve. Multiply the interpolated concentration by the dilution factor to obtain the target protein concentration in the sample.

FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR CLINICAL USE.

